

HEALTH-CHEM DIAGNOSTICS LLC



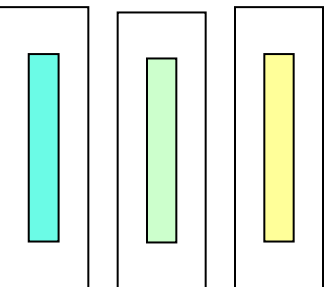
3341 SW 15th St – Pompano Beach, FL 33069 – USA – (954) 979-3845 – Fax: (954) 979-7997 – www.healthchemdiagnostics.com



Enforcement Level - 0.08%

Instructions for use by the Police Department

Product Description

	<p>1. Squeeze middle of the outer plastic tube between thumb and forefinger to break the inner glass ampoule containing yellow crystals. Squeeze only once. Do not crush or bend tube. Use tester immediately.</p>
<p>2. 12 seconds</p> 	<p>2. Each box of 40 test devices contains 4 plastic bags (one per 10 testers), which are used to ensure that enough air passes through the tester. A bag is attached to the tube at the end opposite the blowing end (which is marked with an arrow). Take a deep breath and blow very hard until the bag is fully inflated. Do not inhale. Adequate blowing is indicated by full inflation of the bag which takes approximately 12 seconds. Stop blowing when the bag is fully inflated. Remove it, deflate it, and return it to the kit for additional uses.</p> <p>Note: If the bag cannot be fully inflated in one breath, take a second deep breath and blow again until the bag is full.</p>
<p>2 MINUTES:</p> <p>> 0.08% < 0.08% Negative</p> 	<p>3. After 2 minutes, if the color of the crystals in the tester changes to an Aqua (Green-Blue) cast, the level of alcohol is 0.08% or greater. If the color of the crystals in the tester remains yellow or changes to light Green but not Green/Blue, the alcohol level is below 0.08%. Note: Before reading the results, shake the device to evenly distribute the color of the crystals.</p> <div style="border: 1px solid black; padding: 5px;"> <p>1. GREEN-BLUE: POSITIVE GREATER THAN 0.08%</p> <p>2. LIGHT GREEN: ALCOHOL LEVEL IS LESS THAN 0.08%</p> <p>3. YELLOW: NEGATIVE</p> </div>

Breathcheck® - Breath Alcohol Detector is a disposable breath alcohol indicator designed for one-time use. The Breathcheck® - Breath Alcohol Detector contains indicator chemistry that will undergo a color change in the presence of alcohol contained in the breath of the subject. This product provides a reliable indication of alcohol present in the exhaled breath of the test subject when the instructions for use of the Alcohol \checkmark - Breath Alcohol Detector are rigidly followed.

The device is intended to serve as a screening device for breath alcohol. A positive result requires a confirmation using an evidential quality device.

Use immediately after breaking glass ampoule. Do not use if glass ampoule containing crystals is ruptured prematurely or if crystals are not yellow

The device in this box should not be used after the expiration date printed on the box.

Keep out of reach of children. Do not immerse in liquid.

Do not ingest. If ingested, induce vomiting and contact your physician.

Note: Should not be used in Sodium Vapor Light conditions which could alter the appearance of the color.

Manufactured in the USA by:
HEALTH-CHEM DIAGNOSTICS LLC,
 POMPAÑO BEACH, FLORIDA
 Website: www.healthchemdiagnostics.com



Enforcement Level - 0.08%

Lot Number:

Exp. Date:

NOTE: New improved individual device packaging.

To open without handling mouth piece, so that the device can be assembled and initiated without physically touching the mouth piece end, which comes in contact with the lips.

INSTRUCTIONS:

- 1/ Cut or tear the plastic pouch on the end opposite the mouth piece (mouth piece is indicated by the arrows and the word "blow").
- 2/ Affix the inflation bag to the end of the device (the end containing instructions 1, 2, 3) holding the test by only touching the outside of the plastic pouch.

YOU SHOULD NOW BE READY TO PERFORM THE TEST

- 3/ When ready to perform the test, grip the "Breathcheck - Breath Alcohol Detector" between thumb and forefinger in the approximate area of the window, while still in the protective plastic pouch (See package insert for operating directions).
- 4/ Squeeze to break the ampoule containing the detection crystals. The device may now be removed from the plastic pouch, and handled by the end affixed to the inflation bag, to be placed in the mouth for testing.